

ELITE InGenius



ELITechGroup S.p.A.
C.so Svizzera, 185
10149 Torino ITALY

Offices: Tel. +39-011 976 191 Fax +39-011 936 76 11
E. mail: emd.support@elitechgroup.com
WEB site: www.elitechgroup.com

NOTICE of CHANGE dated 05/05/2022

IMPORTANT COMMUNICATION FOR THE USERS OF PRODUCT:

«ELITE InGenius® SP RNA» Ref. INT034SPRNA

This new revision of the Instruction for Use (IFU) contains the following changes:

- *Update to be in compliance with the Regulation (EU) 2017/746 and the Standard ISO 15223-1:2021 requirements.*

Use and performance of the product remain unchanged.

PLEASE NOTE



LA REVISIONE DI QUESTO IFU E' COMPATIBILE ANCHE CON LA VERSIONE PRECEDENTE DEL KIT



THE REVIEW OF THIS IFU IS ALSO COMPATIBLE WITH THE PREVIOUS VERSION OF THE KIT



CET IFU MIS A JOUR ANNULE ET REMPLACE ET EST PARFAITEMENT COMPATIBLE AVEC LA VERSION PRECEDENTE DU KIT



LA REVISIÓN DE ESTE IFU ES COMPATIBLE TAMBIÉN CON LA VERSIÓN ANTERIOR DEL KIT



A REVISÃO DO ESTE IFU ÉTAMBÉM COMPATÍVEL COM A VERSÃO ANTERIOR DO KIT



DIE REVIEW VON DIESER IFU IST KOMPATIBLE MIT DER VORIGE VERSION VON DEM TEST-KIT

ELITE InGenius

ELITechGroup
EMPOWERING IVD



ELITechGroup S.p.A.
C.so Svizzera, 185
10149 Torino ITALY
Offices: Tel. +39-011 976 191 Fax +39-011 936 76 11
E. mail: emd.support@elitechgroup.com
WEB site: www.elitechgroup.com

ELITE InGenius® SP RNA reagents for Nucleic Acid Extraction


REF INT034SPRNA

ELITE InGenius® SP RNA reagents for Nucleic Acid Extraction

REF INT034SPRNA



IVD



UDI 03661540900075

TABLE OF CONTENTS_Toc433271044

INTENDED USE	1
ASSAY PRINCIPLES	2
MATERIALS PROVIDED	3
MATERIALS REQUIRED BUT NOT PROVIDED	4
OTHER PRODUCTS REQUIRED	5
WARNINGS AND PRECAUTIONS	5
SAMPLES AND CONTROLS	8
PROCEDURE	9
DESCRIPTION OF THE EXTRACTION PROCEDURE	9
PROCEDURE LIMITATIONS	21
TROUBLESHOOTING	22
SYMBOLS	23
NOTICE TO PURCHASER: LIMITED LICENSE	24

INTENDED USE

The «ELITE InGenius® SP RNA» is a cartridge ready-to-use containing reagents for extraction and purification of high-quality total RNA for single test.

«ELITE InGenius® SP RNA» (ELITechGroup S.p.A., code INT034SPRNA) is used in association with the «ELITE InGenius®» (ELITechGroup S.p.A., code INT030) instrument and constitutes, together with ELITechGroup Real Time PCR assays, the **ELITE InGenius System**, fully automated molecular diagnostics systems performing extraction, purification, amplification, detection and results interpretation.

The high-quality total RNA isolation protocol is based on magnetic beads and designed for automated preparation (extraction and purification) from lympho-monocyte suspensions and leukocyte suspensions (~1 x 10⁷ cells) isolated from peripheral blood collected in EDTA or sodium citrate.

«ELITE InGenius SP RNA» does not provide diagnostics results by itself. To obtain diagnostic results, this product must be used with a RNA based amplification assay and **ELITE InGenius System**. The «ELITE InGenius» instrument is intended to perform One-Step Real-Time PCR after RNA extraction. This product is intended for use by professionals such as technicians, physicians and biologists trained in molecular biological techniques. It can be used with downstream assays based on Nucleic Acid Amplification Technologies (NAT assay). The use of this product in association with any downstream diagnostic assay must be validated. Any diagnostic results generated using the extracted nucleic acids in association with any downstream diagnostic assay should be interpreted taking into account other clinical or laboratory findings. Adequate controls for downstream assays should be used in order to mitigate risk of incorrect diagnostic results.

ASSAY PRINCIPLES

The «ELITE InGenius SP RNA» is the reagent set for automated RNA extraction and purification from lympho-monocyte suspensions and leukocyte suspensions isolated from peripheral blood collected in EDTA or sodium citrate of clinical samples in association with the «ELITE InGenius». The reagent set has been optimized for the isolation of nucleic acids from 0.2 mL samples. The resulting nucleic acid extracted is then available for One-Step Real-Time PCR application with «ELITE InGenius».

The RNA isolation process is based on the Magtration® Technology, an automated extraction technology based on magnetic beads, as shown in Figure A below.

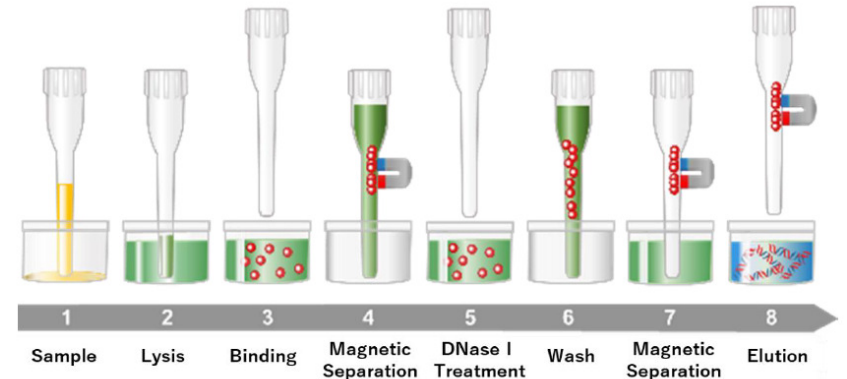


Figure A: Extraction Workflow

The «ELITE InGenius» automatically perform sample dispensing from extraction tubes. The RNA purification procedure is carried out without user involvement, except the initial loading of the instrument, thus allowing safe handling of potentially infectious samples. Sample cross-contamination and reagent cross-over is effectively reduced.

The resulting highly purified nucleic acids are eluted with distilled water. The extraction process on 9 samples takes approximately 75 minutes.

The purified nucleic acids are ready to use for downstream assays based on One-Step Real Time PCR. Otherwise, the purified nucleic acids can be stored at -20 °C or -70 °C for subsequent use.

The kit provides reagents for **48 extractions** (e.g. 16 runs x 3 samples).

Note: The minimum number of samples to be processed per run with the «ELITE InGenius» is 1, the maximum number is 9.

MATERIALS PROVIDED

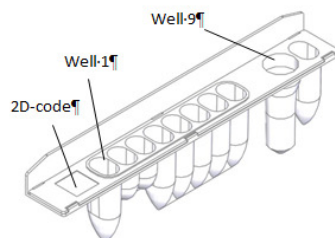


Figure B: Total RNA Extraction Cartridge

The kit contains 48 unitary prefilled Total RNA extraction cartridges.

Each Total RNA extraction cartridge contains:

Well No.	Reagent name	Quantity	H-code/P-code
1	Reductant solution	100 µL	H225, H314, H315, H318, H319, H330, H335, H361, H370, H372, H373, H402, H412
2	PK solution	80 µL	
3	Carrier solution	80 µL	P201, P202, P210, P233, P240, P241, P242, P243, P260, P261, P262, P264, P270, P271, P273, P280, P284, P310, P312, P314, P321, P330, P362, P363, P405, P501
4	Magnetic particles	200 µL	
5	Binding buffer	1200 µL	
6	Wash buffer 1	1200 µL	
7	Wash buffer 2	700 µL	P301+P310, P302+P352, P303+P361+P353, P304+P340, P305+P351+P338, P308+P311, P308+P313, P332+P313, P337+P313, P370+P378, P403+P233, P403+P235
8	Distilled water	1200 µL	
9	Lysis solution	800 µL	

Material Storage

The «ELITE InGenius SP RNA» extraction cartridge should be stored at room temperature (+10 / +30 °C). For the expiration date, please refer to the product label.

Do not freeze. Keep the extraction cartridge away from high temperatures, humidity, and vibration.

Avoid exposure with direct sunlight.

Store the extraction cartridge with the sealed side up.

Material Quality Controls

ELITechGroup S.p.A. (EGSpA) guarantees the performance characteristics of the «ELITE InGenius SP RNA» for applications as described in the manual.

In accordance with the EGSpA certified Quality Management System, the «ELITE InGenius SP RNA» has been tested against established acceptance criteria to ensure consistent product quality.

MATERIALS REQUIRED BUT NOT PROVIDED

The following equipment and reagents are not provided:

- Disposable powder free gloves in nitrile or similar material.
- Laminar airflow hood.
- Micropipettes and sterile tips with aerosol filter or sterile positive displacement tips.
- Vortex mixer.
- Bench microcentrifuge (12,000 - 14,000 RPM).
- Bench centrifuge (3,000 RPM).

Sample tubes for samples are not provided. To run samples on the **ELITE InGenius System**, the user should use the secondary tubes listed below.

Sample Tubes for ELITE InGenius and «BeGenius» Systems

Secondary tubes
Extraction tube (ELITechGroup S.p.A., code INT032CS)

Disposable filter tips and solid waste box are not supplied within the kit. The required consumables are reported below and can be ordered individually from ELITechGroup S.p.A.

Component	Code	Quantity	Description
300 µL Filter Tips Axygen	TF-350-L-R-S	1 box x 10 racks with 96 tips	Standard Volume Tips (300 µL) with filter
ELITE InGenius® Waste Box	F2102-000	20 box / pack	Disposable plastic containers

OTHER PRODUCTS REQUIRED

This product must be used in association with the «**ELiTe InGenius**» instrument (ELiTechGroup S.p.A., code INT030), with the «**ELiTe InGenius® SP 200 Consumable Set**» (ELiTechGroup S.p.A., code INT032CS), and with the «**ELiTe InGenius DNase I**» (ELiTechGroup S.p.A., code INT034DNASE), the «**ELiTe InGenius DNase tube adapter kit**» (ELiTechGroup S.p.A., code G6431-000).

The consumable set, the DNase I and the tube adapter kit can be ordered separately using the code ELiTechGroup S.p.A., code INT032CS, INT034DNASE, G6431-000.

The consumables necessary to carry out the extraction procedure are included in the «**ELiTe InGenius SP 200 Consumable Set**».

The consumable set components are listed below:

Component	Quantity	Description
Extraction tubes	48	Disposable tube to be placed in the extraction position. It can also be used as secondary tube for loading samples
Tip cassettes	4 x 12	Cassette containing a piercing tip and a pipette tip used during the extraction procedure
Elution tubes	50	0.5 mL tube and cap used to collect the extracted Nucleic Acid (NA)

WARNINGS AND PRECAUTIONS

This product is exclusively designed for *in-vitro* use.

General warnings and precautions

Handle and dispose of all biological samples as if they were able to transmit infective agents. Avoid direct contact with the biological samples. Avoid splashing or spraying. All materials that come into contact with the biological samples must be treated for at least 30 minutes with 3% sodium hypochlorite or autoclaved for one hour at 121 °C before disposal.

Handle and dispose of all reagents and all materials used to carry out the assay as if they were able to transmit infective agents. Avoid direct contact with the reagents. Avoid splashing or spraying. Waste must be handled and disposed of in compliance with adequate safety standards.

After receiving the kit, check the kit components for damage. If extraction cartridges are damaged, contact ELiTechGroup Technical Services or your local distributor. In the case of liquid spillage, refer to “Warnings and precautions for specific components” and to the appropriate Safety Data Sheets (SDS).

The chemicals and plastic parts are for laboratory use only; they must be stored in the laboratory and are not to be used for purposes other than intended.

Wear suitable protective clothes and gloves and protect eyes and face.

Discard gloves if they get contaminated.

Never pipette solutions by mouth.

Do not eat, drink, smoke or apply cosmetic products in the work areas.

Carefully wash hands after handling samples and reagents.

Dispose of leftover reagents and waste in compliance with local regulations.

Carefully read all the instructions provided in the product before running the assay.

While running the assay, follow the instructions provided with the product.

Do not use the product after the indicated expiry date.

Do not use damaged kit components.

Only use the reagents provided in the product and those recommended by the manufacturer.

Do not use reagents from other manufacturers.

Warnings and precautions for molecular biology

Molecular biology procedures, such as nucleic acid extraction, amplification and detection, require qualified and trained staff to avoid the risk of erroneous results, especially due to the degradation of nucleic acids contained in the samples or contamination of the samples by amplification products.

The samples must be suitable and, if possible, dedicated for this type of analysis. Samples must be handled in a Class II Biological Safety Cabinet. Pipettes used to handle samples must be exclusively used for this specific purpose and should be cleaned after each use. The pipettes must be of the positive displacement type or be used with aerosol filter tips. The tips used must be both DNase and RNase free, and DNA and RNA free.

Warnings and precautions specific for the components

«**ELiTe InGenius SP RNA**» cartridge is for single use.

The following components of the «**ELiTe InGenius SP RNA**» contain hazardous reagents. GHS Hazard and Precautions statements applied to those components are listed below.

Please, note that hazard labeling is not necessary for quantities less than 125 g or 125 mL.

Lysis Solution

Contains Guanidinium thiocyanate and Sodium N-lauroylsarcosinate



Danger

H314: Causes severe skin burns and eye damage

H315: Causes skin irritation.

H318: Causes serious eye damage

H330: Fatal if inhaled

H412: Harmful to aquatic life with long-lasting effects

P260: Do not breathe dust/fumes/gas/mist/vapours/spray.

P262: Do not get in eyes, on skin, or on clothing.

P264: Wash the hands thoroughly after handling.

P270: Do not eat, drink or smoke when using this product.

P271: Use only outdoors or in a well-ventilated area.

P273: Avoid release to the environment.

P280: Wear protective gloves/protective clothing/eye protection/face protection.

P284: Wear protective gloves/protective clothing/eye protection/face protection.

P301+310: IF SWALLOWED: Immediately call a POISON CENTER/doctor.

P301+P330+P331: IF SWALLOWED: Rinse mouth. Do NOT induce vomiting.

P302+P352: IF ON SKIN: Wash with plenty of water.

P303 + P361 + P353: IF ON SKIN (or hair): Take off immediately all contaminated clothing. Rinse skin with water/shower.

P304+P340: IF INHALED: Remove person to fresh air and keep comfortable for breathing.

P305+P351+P338: IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing.

Immediately call a POISON CENTER/doctor.

P310: Specific treatment.

P321: Rinse mouth.

P330: Rinse mouth.

P332+P313: If skin irritation occurs: Get medical advice/attention.

P362: Take off contaminated clothing.

P363: Wash contaminated clothing before reuse.

P403+P233: Store in a well ventilated place. Keep container tightly closed.

P405: Store locked up.

P501: Dispose of contents/container according to national regulation.

ELiTe InGenius® SP RNA
reagents for Nucleic Acid Extraction

REF INT034SPRNA

Binding Buffer Wash Buffer 1, and Wash Buffer 2

Contains 2-propanol



Danger

- H225:** Highly flammable liquid and vapour.
H319: Causes serious eye irritation.
H335: May cause respiratory irritation.
H361: Suspected of damaging fertility or the unborn child.
H370: Causes damage to organs.
H372: Causes damage to organs through prolonged or repeated exposure.
H373: May cause damage to organs through prolonged or repeated exposure.
- P201:** Obtain special instructions before use.
P202: Do not handle until all safety precautions have been read and understood.
P210: Keep away from heat, hot surfaces, sparks, open flames and other ignition sources. No smoking.
P233: Keep container tightly closed.
P240: Ground/bond container and receiving equipment.
P241: Use explosion-proof electrical/ventilating/lighting equipment.
P242: Use only non-sparking tools.
P243: Take precautionary measures against static discharge.
P260: Do not breathe dust/fumes/gas/mist/vapours/spray.
P261: Avoid breathing dust/fume/ gas/mist/vapours/spray.
P264: Wash the hands thoroughly after handling.
P270: Do not eat, drink or smoke when using this product.
P271: Use only outdoors or in a well-ventilated area.
P280: Wear protective gloves/protective clothing/eye protection/face protection.
P303+P361+P353: IF ON SKIN (or hair): Take off immediately all contaminated clothing. Rinse skin with water/shower.
P304+P340: IF INHALED: Remove person to fresh air and keep comfortable for breathing.
P305+P351+P338: IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing.
P308+P311: If exposed or concerned: Call a POISON CENTER or a doctor.
P308+P313: If exposed: Call a POISON CENTER or a doctor.
P312: Call a POISON CENTER or a doctor if you feel unwell.
P314: Get medical advice/attention if you feel unwell.
P321: Specific treatment.
P337+P313: If eye irritation persists: Get medical advice/ attention.
P370+P378: In case of fire: use carbon dioxide, foam, dry chemical and water fog to extinguish.
P403+P233: Store in a well-ventilated place. Keep container tightly closed.
P403+P235: Store in a well ventilated place. Keep cool.
P405: Store locked up.
P501: Dispose of contents/container according to national regulation.

Reductant Solution

Contains sodium dodecyl sulfate



Danger

- H315:** Causes skin irritation
H318: Causes serious eye damage
H319: Causes serious eye irritation.
- P264:** Wash the hands thoroughly after handling.
P280: Wear protective gloves/protective clothing/eye protection/face protection.
P362: Take off contaminated clothing and wash before reuse.

ELiTe InGenius® SP RNA
reagents for Nucleic Acid Extraction

REF INT034SPRNA

- P302+P352:** IF ON SKIN: Wash with plenty of soap and water.
P305+P351+P338: IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing.
P332+P313: If skin irritation occurs: Get medical advice/attention.
P337+P313: If eye irritation persists: Get medical advice/ attention.

For further information, please, see Material Safety Data Sheets.

No other component of the «**ELiTe InGenius SP RNA**» contains hazardous reagents that require European Community Risk and Safety phrases and GHS Hazard and Precautions phrases.

Do not reuse extraction cartridge or tip rack.

Do not damage or obscure the 2D code.

When liquid drops are present on the wall of the cartridge well, shake gently without creating bubbles to move the drops down to the bottom of the tube.

Elution is performed with distilled water, the eluate final volume may be affected by residues on the magnetic beads, on the tip surface or evaporation.

The use of an internal control is recommended to obtain reliable diagnostic results.

Warnings and precautions specific for ELiTe InGenius System

In the case of an instrument error message, please refer to instrument Operator's Manual (ELiTechGroup S.p.A., code INT030).

SAMPLES AND CONTROLS

For reproducible and high yields of extraction, appropriate sample collection, transport and storage is essential. Yields may vary from sample to sample depending on factors such as the patient, the sample age and the type of sample.

EDTA or sodium citrate, can be used to collect the samples to be used with the «**ELiTe InGenius SP RNA**».

Note: Samples should not contain clots or other solid materials. Mix the sample to ensure a homogenous resuspension before loading onto the instrument.

Peripheral blood collected in EDTA or sodium citrate

The peripheral blood collected in EDTA or sodium citrate, used for RNA extraction, must be collected according to laboratory guidelines, transported at +2 / 8 °C and stored at +2 / 8 °C for a maximum of 48 hours prior to purification.

Do not freeze peripheral blood in order to prevent degradation of RNA.

When starting with peripheral blood it is advisable to separate leukocyte according to laboratory guidelines.

Interfering substances

Whole blood samples **must not contain heparin**, as it is a powerful inhibitor of DNA polymerase enzymes (such as thermostable DNA polymerases and reverse transcriptase) and leads to invalid or incorrect results in downstream assays performed on the extracted RNA.

Any inhibitory effect caused by drugs that may be contained in the starting sample will have to be evaluated each time by the user in account of downstream assays performed on the extracted RNA.

Extraction quality controls

Extraction quality controls may be used for training, proficiency testing and external QC of the System. External controls may be used in accordance with guidelines or requirements of local regulations or accreditation organizations.

As a negative specimen processing control, the laboratory can use a negative sample that has already been tested with the downstream assay or carry out a simulated extraction using molecular biology grade water in place of the sample.

As a positive specimen processing Control, the Laboratory can use a positive sample that has already been tested with the downstream assay or a certified reference material.

PROCEDURE

Read the «ELiTe InGenius» operator's manual carefully.

PREPARATION OF SAMPLES

Transfer 10 – 14 mL of fresh peripheral blood collected in EDTA or sodium citrate into a 15 mL tube after mixing it thoroughly by inversion. Centrifuge for 10 minutes at 3000 RCF; add 5 mL of Cell Lysis Solution (Promega, Ref. A7933) into a new 15 mL tube; with a 1 mL pipette, remove the buffy-coat obtained after centrifugation and transfer it to the 15 mL tube containing the lysis solution; aspirate and release until the cells are inside the tube and the pipette is free of material; incubate at room temperature for 10 minutes and mix by inversion (NO VORTEX) at least 3-4 times; centrifuge at 3000 RCF for 10 minutes; remove the supernatant and resuspend in 2 mL of Cell Lysis Solution by transferring it into a 2 mL tube; centrifuge again for about 2 minutes at 3000 RCF; carefully remove the supernatant and resuspend the pellet in 200 µL of Lysis Solution (1 mL of Lysis Buffer, Promega, Ref. Z3051 + 20 µL of 1-Thioglycerol, Promega, Ref. A208B-C).

Samples must be transferable by pipette; ensure there are no clots or other solid materials.

Volume of samples in the Extraction tubes

The pre-treated sample can be directly loaded into the system using the extraction tubes («ELiTe InGenius SP 200 Consumable Set», ELiTechGroup S.p.A., code INT032CS).

DESCRIPTION OF THE EXTRACTION PROCEDURE

Extraction with the «ELiTe InGenius SP RNA» reagent cartridge is performed automatically by the ELiTe InGenius System. The procedure includes the following steps:

1. Switch on the instrument.
2. Select functions from the system screen. It is possible to perform a session for "Extraction Only" or "Extraction plus PCR".
3. Select the assay to be run.
4. Put the total RNA extraction reagent cartridge, DNase I, DNase I tube adapter, tip set included in the consumable set, and sample in positions as indicated on the GUI.
5. Examine if the reagent sticks to the interior wall of the cartridge before use. Shake lightly to allow the drops to fall without making bubbles. If DNase I powder sticks to the cap or interior wall of the vial, spin down briefly. Make sure to put DNase I into the DNase I tube adapter and remove the cap before placing into the instrument.

Reagent and consumable required for one sample extraction are listed as follows. Put them into the instrument according to the GUI guidelines of the instrument.

- | | |
|-----------------------------------|------|
| - ELiTe InGenius SP RNA cartridge | 1 pc |
| - DNase I | 1 pc |
| - DNase I tube adapter | 1 pc |
| - Tip set | 1 pc |
| - Elution tube | 1 pc |
| - Extraction tube | 1 pc |

6. Close the instrument front cover.
7. Push Start button to start the total RNA extraction process.
8. After process completion, open the front cover by following prompts on the system screen. Extracted RNA will be used directly in PCR reaction if a full "Extraction plus PCR" method was selected. If "Extraction plus PCR" was not selected, the extracted RNA may also be stored in the 0.5 mL elution tube. After the run, tighten the screw cap and store the sample for future use.

General overview of the ELiTe InGenius working area

The ELiTe InGenius System has been developed and validated for specific *in-vitro* diagnostic (IVD) applications by ELiTechGroup S.p.A. in combination with IVD extraction kits and IVD Real Time PCR kits.

An overview of the «ELiTe InGenius» instrument is shown in Figure 1.

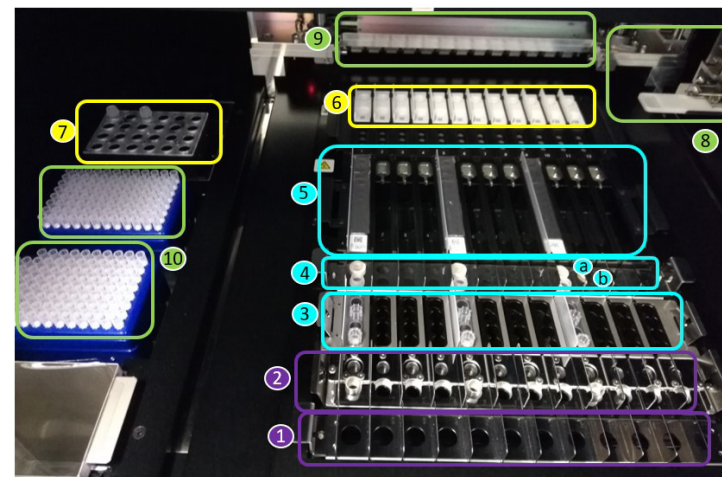


Figure 1: The «ELiTe InGenius» loading area

Figure 1 shows: Primary tube rack position (1), Extraction tube rack position (2), Tip rack position (3), Elution tube rack position (Dnase I tube + tube adapter (a) and Elution tube (b)) (4), Extraction cartridge rack position (5) and PCR cartridge rack position (6), PCR and Internal Control reagent block (inventory manager) position (7), sample and reagent dispensing (8, 9), the waste box (left-bottom) and tips positions (10).

The single head pipettor (8) starting positions is in the right back of the machine. All movable parts work only when the «ELiTe InGenius» instrument is closed and locked.

Loading of the «ELITE InGenius» instrument

Refer to the «ELITE InGenius» operator’s manual.

Switch on the «ELITE InGenius» instrument using the power switch located on the right side of the instrument. The «ELITE InGenius» instrument software will be automatically loaded after the system has booted up. Please keep the door of the instrument system closed during system initialization.

Instrument set-up

After logging in by "Open" or "Close" modality (IVD certified), the main screen "Home" appears (Figure 2).

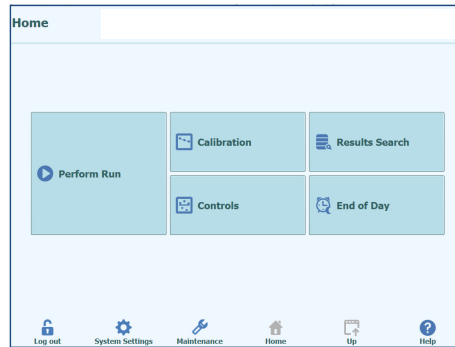


Figure 2: «ELITE InGenius» Home screen

1. Select "Perform Run" to start loading the system and prepare for starting a run.

The Perform Run screen appears (Figure 3).



Figure 3: "Perform Run" screen

"Input Volume" (Treated Volume) depends on the extraction reagents. The volume of treated sample is 200 µL.

"Elute Volume" depends on specific assays. Possible elution volumes are 50, 100, 200 µL.

Sample ID (SID) and Assays to be performed must be specified. The picture below shows an example (Figure 4).

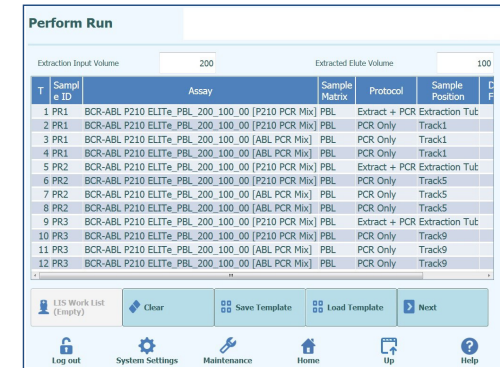


Figure 4: Example of Sample ID and Assay specification

2. Select "SID". Enter the sample ID using the keypad or barcode scanner.
3. Select "Assay". Choose the assay from the list.

The system screen will be updated according to the assay selected.

4. Select "Protocol" to define "Extraction only" or "Extraction plus PCR" methods.

At this point, sample positions can be saved to create a panel template. For instructions on how to save the settings refer to the «ELITE InGenius» operator’s manual.

Note: with ELITE InGenius SP RNA kit, samples can only be loaded into the Extraction tube.

5. Press the "Next" button to proceed with the disposable-loading.

The "Load / Unload Inventory" screen appears (Figure 5).

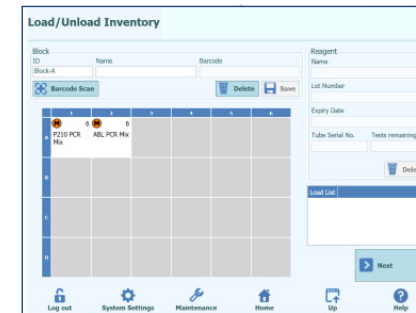


Figure 5: "Load / Unload Inventory" screen

This screen allows the user to confirm reagent and control loading according to the settings defined in the "Perform Run" screen.

6. To confirm that sufficient reagents for the number of tests selected are placed in the inventory manager position 7 (cfr. page 10, Figure 1) as indicated on the screen, press the "Next" button.

Note: "Next" button is enabled when there are sufficient reagents/controls for the run.

The "Load / Unload Inventory" screen for Tip rack loading appears (Figure 6).

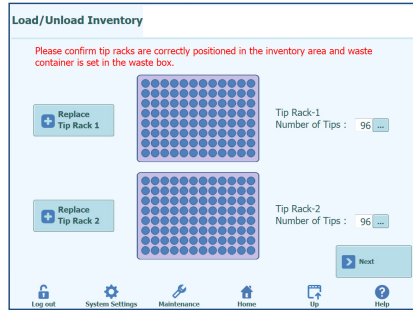


Figure 6: The "Load / Unload Inventory" screen confirms tip rack placement

7. Place sufficient Tips racks in position 10 (cfr. page 10, Figure 1).
8. Press the "Next" button.

Note: The "Next" button will not be enabled until there are sufficient Single Tips loaded for the run.

The "Disposable" screen appears to guide the user during the disposables loading. The first screen is related to the PCR Rack loading (Figure 7).

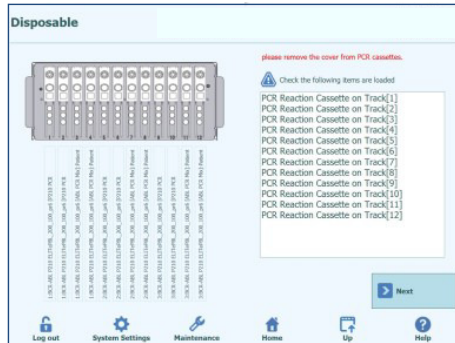


Figure 7: The "Disposable" screen is used to confirm loading PCR racks

When "Extraction plus PCR" Protocol has been selected in the "Perform Run" screen:

9. Place the PCR cassettes indicated in position 6 (cfr. page 10, Figure 1).
10. Press the "Next" button.

Note: If the Extraction only protocol was selected in the "Perform Run" screen, the PCR Cassette don't have to be loaded.

The "Disposable" screen for Extraction Rack loading with Extraction Cartridge appears (Figure 8).

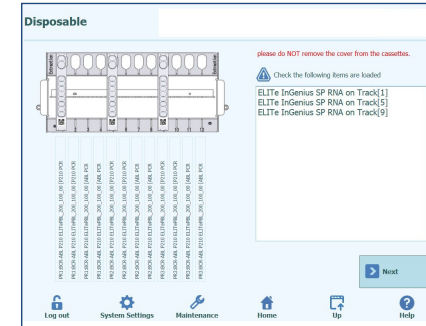


Figure 8: The "Disposable" screen is used to confirm Extraction Rack loading

11. Place the Extraction cartridge cassette(s) indicated in position 5 (cfr. Page 10, Figure 1).
12. Press the "Next" button.

Note: The "Next" button is enabled when there is sufficient number of Extraction cartridge for the run are loaded.

The "Disposable" screen for DNase I, into the DNase I tube adapter, loading with Elution Tube Rack appears (Figure 9).

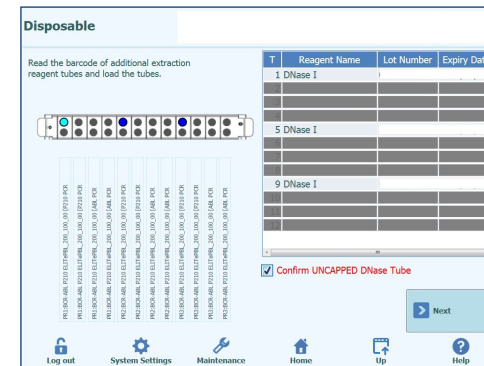


Figure 9: The "Disposable" screen is used to confirm loading of DNase I in Elution Tube Rack

13. Place the DNase I, into the DNase I tube adapter, indicated in position 4 (cfr. Page 10, Figure 1).
14. Press the "Next" button.

The “Disposable” screen for elution tube loading with Elution Tube Rack appears (Figure 10)


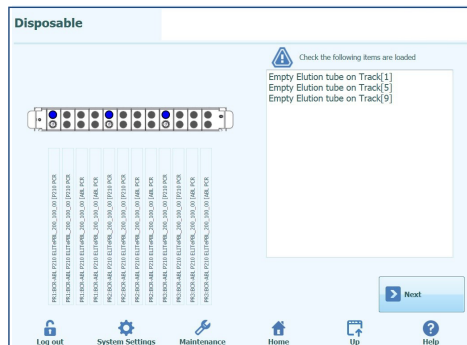


Figure 10: The “Disposable” screen is used to confirm loading of Elution Tube Rack with elution tube

15. Place the amount of elution tubes, indicated in position 4 (cfr. page 10, Figure 1).
16. Press the “Next” button.

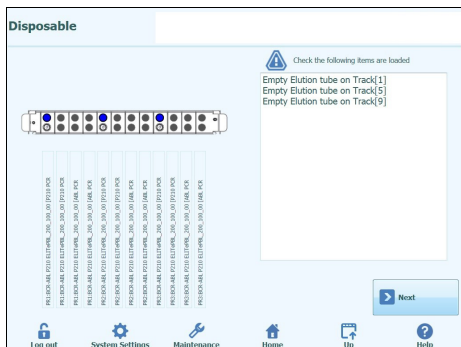

The “Disposable” screen for tip rack loading appears (Figure 11).

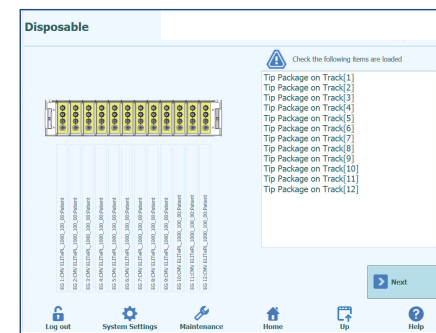


Figure 11: The “Disposable” screen is used to confirm loading tips racks

17. Place the amount of Tip cassettes indicated in position 3 (cfr. page 10, Figure 1).

Ensure that the Tip (1) and the piercer (3) are placed as shown in the picture below (Figure 12).




Figure 12: Tips disposition on Tip Cassette

18. Press the “Next” button.

The “Disposable” screen for extraction tube rack loading appears (Figure 13).

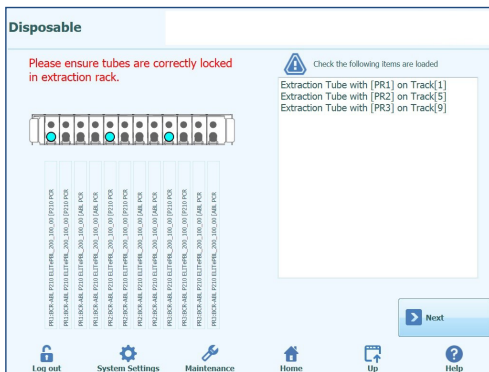


Figure 13: The “Disposable” screen is used to confirm loading extraction tube racks

19. Place the amount of extraction tubes indicated in position 2 (cfr. page 10, Figure 1).
20. Press the “Next” button.

Note: 200 µL of the sample must be present in the “Extraction Tube”.

The “Disposable” screen for sample rack loading appears (Figure 14).

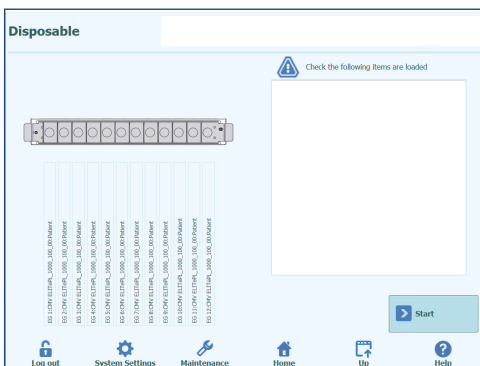


Figure 14: The “Disposable” screen is used to confirm loading of sample racks.

21. Press the “Start” button to start the run.

The following message is shown (Figure 15).

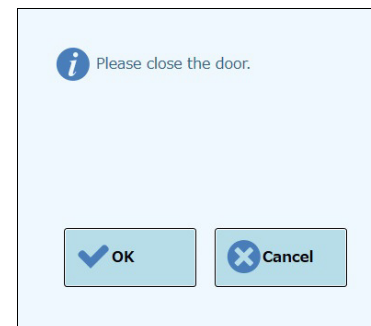


Figure 15: Instrument close door request message

22. Close the front door and press the “OK” button on the popup message.

The “During Run” screen appears (Figure 16). The run process can be followed on this screen.



Figure 16: During run screen

End of Assay:

If an "Extraction plus PCR" protocol was selected, the "End of Run" screen is shown. The "OK" button becomes active when the instrument front door may be opened (Figure 17).

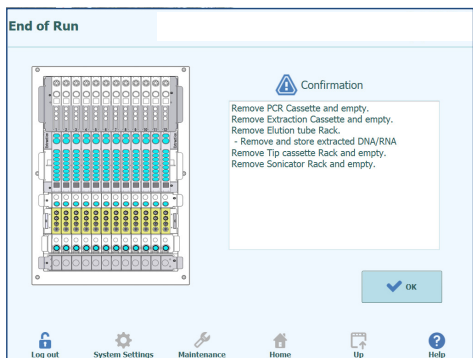


Figure 17: The End of Run screen

23. Open the front door.

Instructions to unload, store or discard samples, materials and reagents are listed in the "End of Run" screen.

24. Carry out the actions listed immediately.

25. To confirm all actions have been completed, press "OK".

The extracted RNA may be stored at -20 °C for a maximum of thirty days or at -70 °C for longer periods. Freeze/Thawing cycles of extracted RNA must be limited to 5 times in order to avoid titre loss.

As with other diagnostic equipment, all waste products (liquids, tips, tubes and cartridges) should be treated as potentially dangerous bio-hazardous waste and discarded accordingly.

Shutdown of System:

26. On the Home screen, select "End of Day". The following screen is shown (Figure 18).

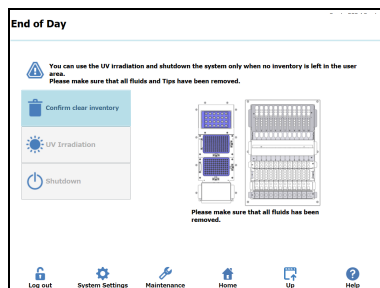


Figure 18: End of Day screen

27. Verify that the user area has been unloaded.

28. Press "Confirm clear inventory" button. The elimination of the reagents is saved in the system that will then allow shutdown to be executed.

Daily maintenance (UV decontamination):

The «ELITE InGenius» instrument is equipped with an internal UV lamp (254 nm wavelength) that should be used daily, either at the end of the working day or in the morning before any run is started. The suggested decontamination time is about 30 min.

1. To start UV decontamination, on the home screen of the «ELITE InGenius» instrument, select "End of Day" and then press "UV Irradiation".

Following message is displayed (Figure 19):




Figure 19: The Close door request message

2. Close the front door and press "OK".

A message is displayed to allow the choice of automatic shutdown after irradiation (Figure 20).

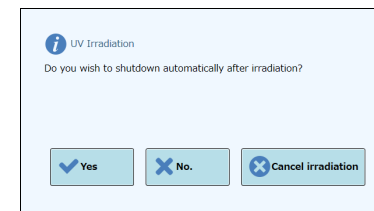


Figure 20: Choice of automatic shutdown after irradiation message

3. Select the desired option. Irradiation will be started.

As irradiation is performed, a status screen will be displayed showing the progress of the process.

PROCEDURE LIMITATIONS

Only use the following clinical samples with this product: lympho-monocyte suspensions and leukocyte suspensions isolated from peripheral blood collected in EDTA or sodium citrate. The kit validation is limited to the matrices mentioned in the intended use, other matrices leads to loss of compliance with Regulation IVDR (EU) 2017/746 for the respective process. No guarantee is issued with differing sample type or change in the procedure.

This product is in compliance with the Regulation IVDR (EU) 2017/746 for *in-vitro* medical devices. In-vitro diagnostic use of the product in countries where the Regulation IVDR (EU) 2017/746 is not recognized may be subjected to the fulfilment of registration procedures according to local competent authorities.

The user is responsible to validate the performance of the product if used with assays different from those validated by ELiTechGroup S.p.A. as reported in the instructions for use. ELiTechGroup S.p.A. does not provide validation of performance characteristics of the product regarding these applications.

The product may be used in a clinical laboratory if the laboratory diagnostic system has been validated as per EN ISO 15189 in European countries or equivalents in other countries.

Do not use whole blood samples collected in heparin with this product. Heparin inhibits DNA polymerase enzymes (such as thermostable DNA polymerases) and leads to invalid or incorrect results in subsequent steps of the analysis performed on the extracted nucleic acids.

Any inhibition phenomena from drugs that may be present in the starting sample may be evaluated in the extraction product depending upon how the extraction product is used.

The results obtained with this product are subject to the correct identification, collection, transport, storage and preparation of samples. To avoid incorrect results it is necessary to take particular care during these activities and to carefully follow the instructions provided.

This product must be handled by personnel qualified and trained in the processing of potentially infective biological samples and dangerous chemical preparations in order to prevent accidents with potentially serious consequences for the user or other persons.

This product requires the use of work clothes and work areas that are suitable for the processing of potentially infective biological samples and dangerous chemical preparations to prevent accidents with potentially serious consequences for the user or other persons.

This product must be handled by personnel qualified and trained in molecular biology techniques, such as extraction, amplification and detection of nucleic acids, to avoid incorrect results with potentially serious consequences for the patient in subsequent steps of the analysis performed on the extracted nucleic acids.

This product must be handled in separate areas for extraction / preparation of amplification reactions and for amplification / detection of amplification products to avoid false positive results with potentially serious consequences for the patient in subsequent steps of the analyses performed on the extracted nucleic acids.


This product requires the use of special clothing and instruments for extraction, preparation of amplification reactions and for amplification / detection of amplification products to avoid false positive results with potentially serious consequences for the patient in subsequent steps of the analysis performed on the extracted nucleic acids.

TROUBLESHOOTING


Problem	Probable Cause	Comments and Suggestions
Low yield of extraction or RNA purity	Sample status	Verify that the sample storage condition is appropriate as reported in the sample and controls section. Use only fresh sample or sample stored under appropriate conditions. Extraction yield can vary from fresh or frozen sample.
	Reagent status	Verify that the extraction reagent cartridge storage condition is appropriate. Do not freeze the reagents and avoid storage locations subject to vibration.
	Solid items residues	Sample extracts with solid residues may cause tip obstruction, and the mixing process may not function properly. The sample should be an homogeneous solution for smooth handling by the 1000 µL pipet. Do not use solids in samples to be extracted.
	Issues with automation system	Refer to the error code displayed in the instrument operator's manual.
Contaminated extracts	Contamination with DNA or RNA	Clean carefully all instrument components and surfaces after use, using an agent capable of eliminating DNA and RNA.
RNA is degraded	Sample concentration too high	If an high concentrated sample has used, the RNase cannot be inactivated. Dilute sample before loading.
	Elution storage	Do not store eluate at RT for long time. Tighten cap of elution tube as soon as possible, and keep samples at -20 °C.
	External RNase contamination	After use, clean all parts on the instrument surface carefully by using RNase removal agents.

SYMBOLS


REF Catalogue Number

 Temperature limits


LOT Batch code


 Use by (last day of month)


IVD *In vitro* diagnostic medical device

 Fulfilling the requirements of the Regulation IVDR (EU) 2017/746 for *in vitro* diagnostic medical device


UDI Unique Device Identification

 Contains sufficient for "N" tests


 Do not reuse


 Consult instruction for use

CONT Contents


 Keep away from sunlight


 Manufacturer

 Country of manufacture

 Health Hazard

 Danger

 Flammable

 Corrosive

NOTICE TO PURCHASER: LIMITED LICENSE

ELITE InGenius® technology is covered by patents and requests for patents.

This limited license allows the person or entity to whom the product has been provided to use the product and data generated with the use of the product, only for human diagnostics. Neither ELITechGroup S.p.A. nor its licensors grant other explicit or implied licenses for other purposes.

Magtration® is a registered trademark owned by Precision System Science Co., Ltd.

ELITE InGenius® is a registered trademark of ELITechGroup.